

HTRF® Research Reagents

HTRF Human IFN g kit - 500 pts

Product Number : 62HIFNGPEG Lot Number : 16A


Expiration date : 2028-02-03 Document version : 1

Reagents :	Lot n°
HTRF Diluent 5 (5X) - 2 mL	22B
HTRF Detect. Buf. 3 - 1.5 mL	31A
HTRF Human IFN g kit - Std	14A
HTRF Human IFN g kit - 500 pts Eu Cryptate antibody	16A
HTRF Human IFN g kit - 500 pts XL665 antibody	15A
/	/

Results :

Incubation : Overnight at RT
 Plate : 384 wells small volume white plate 20 µL
 Reader : Envision
 Fitting model : 4 Parameter Logistic (4PL 1/y2)* model

hIFNg	Conc. (pg/ml)	DF %	DF Accepted Range
Std 1	46,6	21%	13-21
Std 2	98	40%	25-48
Std 3	205,7	77%	60-96
Std 4	432	150%	129-195
Std 5	907	281%	263-387
Std 6	1904,8	645%	556-747
Std 7	4000	1027%	1026-1310

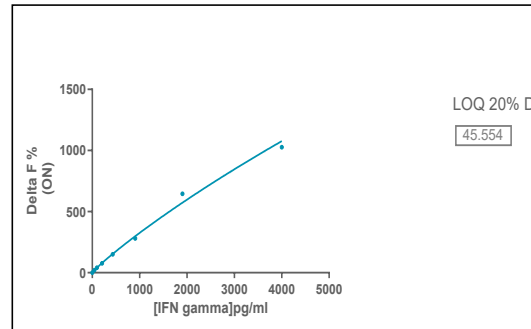

Assay characteristics :

	Found value	Specifications Rev 01
Detection limit	9 pg/ml	≤ 15 pg/ml

HTRF Human IFN g kit - 500 pts - Lot n° : 16A

Accepted

Rejected

Quality control date : 2025-09-30	Supervisor's initials : MP
-----------------------------------	----------------------------

The information provided in this document is valid for the specified lot number and date of analysis. This information is for reference purposes only and does not constitute a warranty or guarantee of the product's suitability for any specific use. Revvity, Inc., its subsidiaries, and/or affiliates (collectively, "Revvity") do not assume any liability for any errors or damages arising from the use of this document or the product described herein. REVVITY EXPRESSLY DISCLAIMS ALL WARRANTIES, INCLUDING WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE, REGARDLESS OF WHETHER ORAL OR WRITTEN, EXPRESS OR IMPLIED, ALLEGEDLY ARISING FROM ANY USAGE OF ANY TRADE OR ANY COURSE OF DEALING, IN CONNECTION WITH THE USE OF INFORMATION CONTAINED HEREIN OR THE PRODUCT ITSELF.